



Rechargeable Battery

LinkVieW The test solution of Energy Storage Device

Combining DC regulated power supply and electronic load device, charge / discharge test is easily started with LinkVieW.


GW Instek introduces LinkVieW software to allow users to quickly set test instruments for the operation of charging and discharging tests on battery and super capacitor, etc. Users can define charging and discharging procedures to automatically execute procedures so as to obtain measurement results. History graphs are available and they can be exported to Excel for further analysis.

● テストイメージ

Test Image

※1 Interface setting depend on the each model.


The Automatic charging and discharging test of Energy Storage Device Up to 12 channels

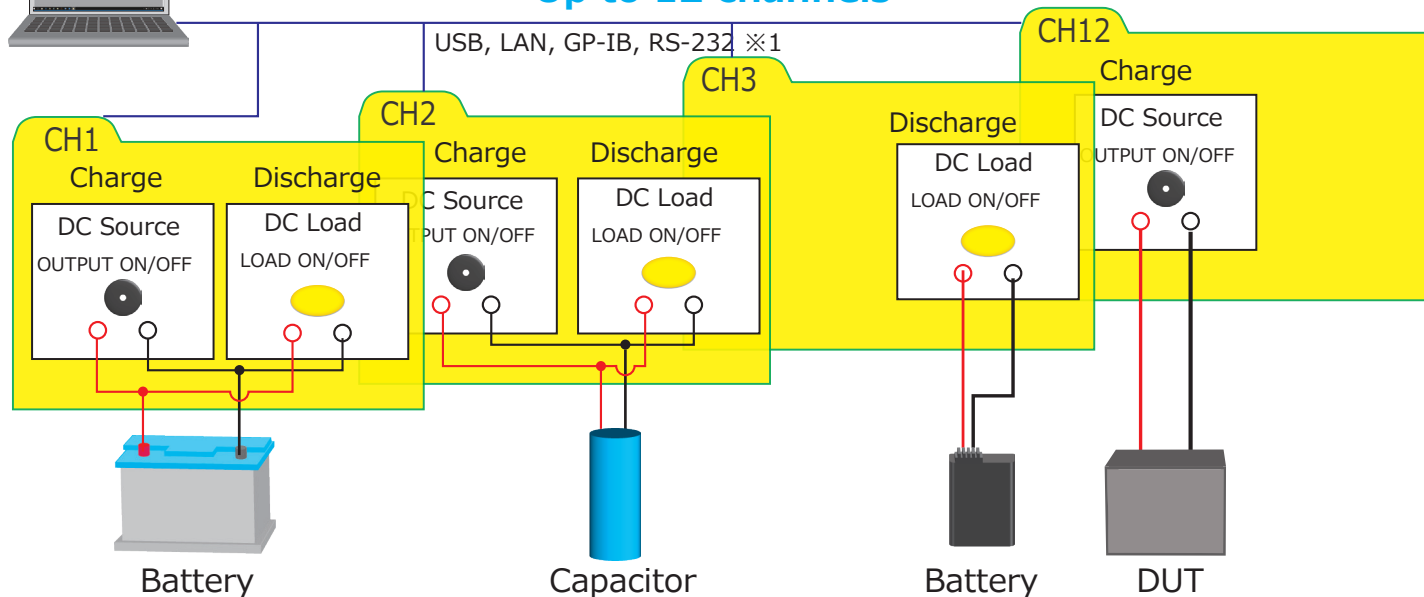


● Device setting

● Edit : Charging / Discharging procedure editing


● Test : Start/Stop

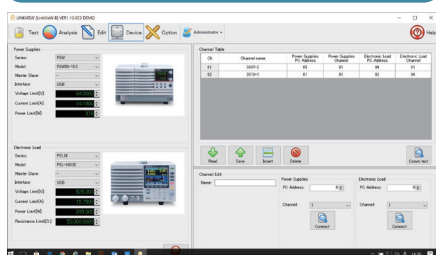

Up to 12 channels

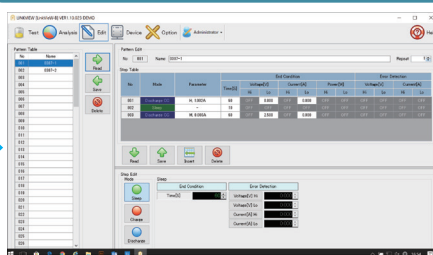

Support up to 100 patterns (sequence).
Sequence steps: 1000 steps Max.
Minimum record period: 1s. ※2
Maximum step time: 100 Min.
Maximum repeat cycles: 65535 cycles.

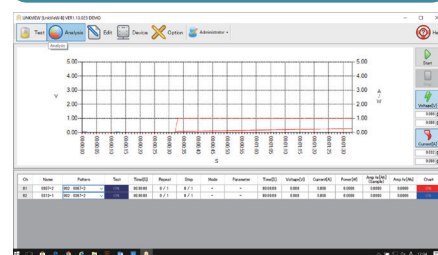


● Feature

✓ Easily expand capacity.

- Long Term Power Monitoring of I, V, P(W)
- Create/define operation sequence for controlling Source/Load behavior.
- Simultaneously run test sequence of each channel and data logging
- Data Analyzer:
- VIEW chart: support Zoom In/Tracking of Samples
- VIEW table: summaries testing result for VIEW and also each step including Voltage/Current/Power/VMax/Imax/PMax/AmpHour
- Live Data Monitoring:
- VIEW: Self-defined display range/offset adjustable
- Controllable displayed Graph setting


● Analysis ※3

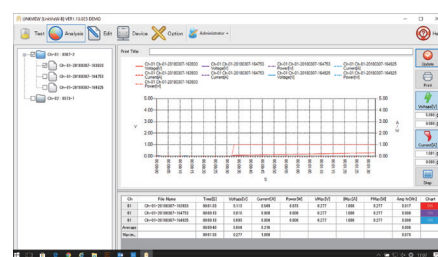

※2 If the number of channels to be examined will increase, the sampling time per channel will increase due to the communication time

※3 LinkVieW trial version doesn't work Data Log and Analysis function.

Device Setting (Channel setting)

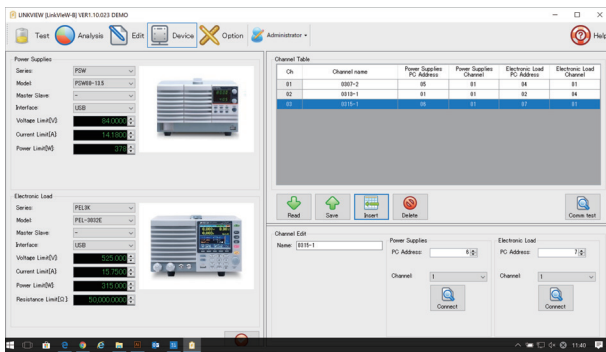

Up to 12 channels

Edit channel

You can select used devices for each channels at 'Edit' button in the tool bar.

You can also set from One channel up to Twelve channels.

* 'Channel' also can consist one Power supply or one Electronic Load.

Support Models:


DC Power supply : PSU series / PSW series / PSB series



DC Load : PEL-3000 series / PEL-3000E series / PEL-2000A series



Edit : Charging / Discharging procedure editing

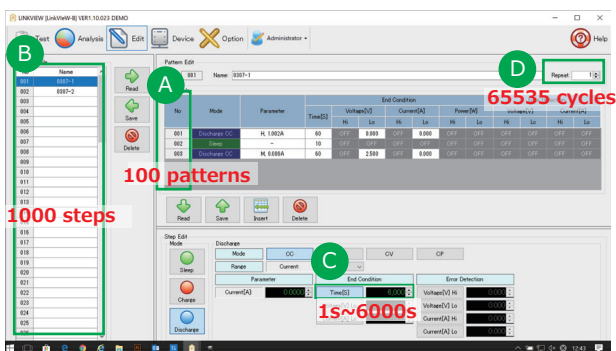

You can set Examination pattern; Charge, discharge and Sleep.



(1) Sleep : End Condition (time [s])

Error Detection Hi/Lo Voltage and current



(2) Charge : Setup the power supply

Voltage, current, End Condition and Error Detection.



(3) Discharge : Setup the parameters of electronic load

Mode ; CC, CR, CP, CR, etc.

Range ;


Parameter;

End Conditions ; Discharge Time, Voltage and Current.※1

Error Detection ;Error will be detected when the over/under setting voltage or current is detected

※1: Priority is given to the contents to which end conditions are met first.

Test : Start/Stop

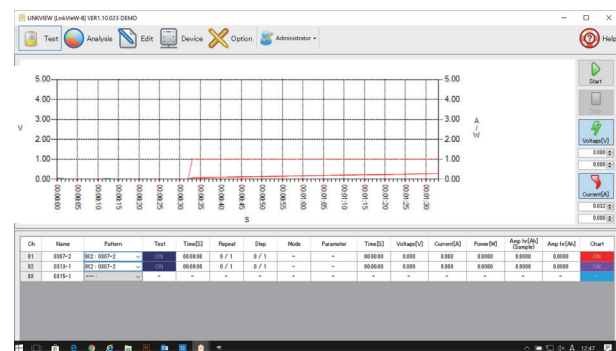

Click 'Start' button and examination will begin.

Graph will be displayed on the second.



When you suspend all the examinations on the way, click 'Stop' button. All the examinations will stop irrespective of the situation of each channel.

Ch	Name	Pattern	Test	Time	Repeat	Step	Mode	Parameter	Time	Voltage	Current	Power	App. Ir (A)	App. Ir (A)	Chart
01	0007-2	002 0007-2	ON	00:00:00	0 / 1	0 / 1	-	-	00:00:00	0.000	0.000	0.000	0.0000	0.0000	ON
02	0010-1	002 0007-2	ON	00:00:00	0 / 1	0 / 1	-	-	00:00:00	0.000	0.000	0.000	0.0000	0.0000	ON
03	0010-1	002 0007-2	ON	00:00:00	0 / 1	0 / 1	-	-	00:00:00	0.000	0.000	0.000	0.0000	0.0000	ON

Name : Select Channel Name


Pattern : Select Patarn Name

Test : Select ON or OFF


Chart : Select ON or OFF at Disply.

Other condition are depend on pattern settings.

Analysis ※3

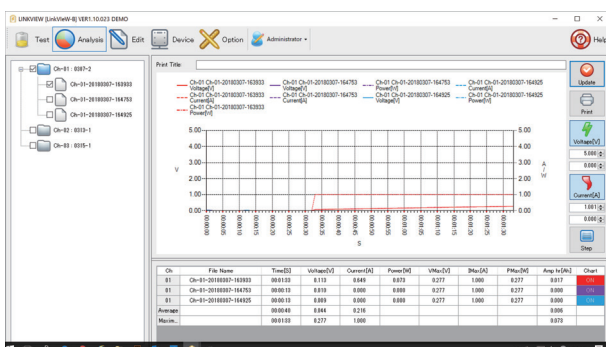

The data acquired by the examination can be checked on an analysis screen. Click 'Analysis' button and an analysis screen will be displayed.



It is a folder of channel 1 (test1).

The first test data is contained.

The second test data is contained.

It is a folder of channel 2 (test2).

A data folder is created in a channel folder.



One data folder will be created for every examination.



Click 'Updating' button after choosing the data, a graph and data will be displayed. A graph is classified by color for every data.

* Since the graph of current is displayed in an absolute value, it becomes a plus direction irrespective of charge and discharge.

8 channel Charge / Discharge Test

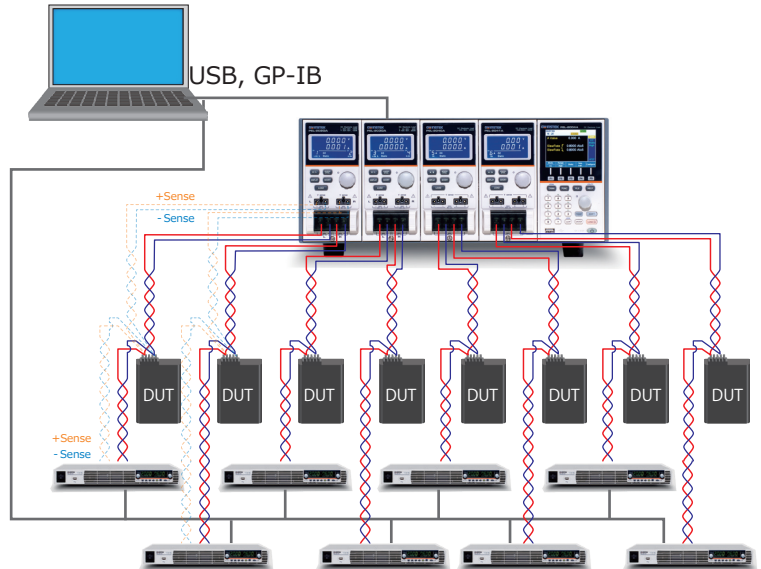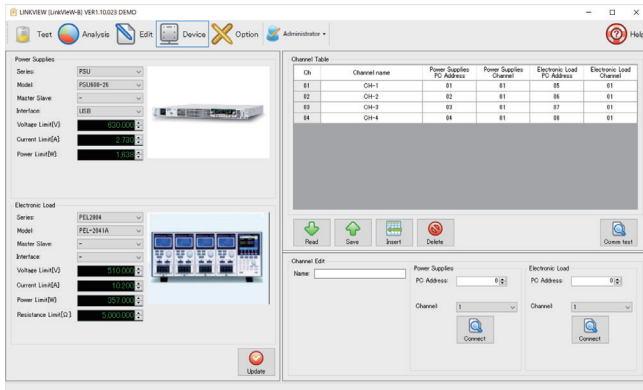

PEL-2000A series

D.C. Electronic Load Mainframe

PEL-2002A: 2 Slot PEL-2004A : 4 slots



Interface : USB, RS-232, GPIB(Optional)


D.C. Electronic Load Module

PEL-2020A PEL-2030A PEL-2040A PEL-2041A



100W × 2 ch 2ch 1ch 1ch
30W, 250W 350W 350W

Load Module	Description
PEL-2020A	200W, Dual Channel Module, (0~80V, 20A, 100W) x2
PEL-2030A	280W, Dual Channel module, (1~80V, 5A, 30W) & (1~80V, 40A, 250W)
PEL-2040A	350W, Single Channel, (0~80V, 70A, 350W)
PEL-2041A	350W, Single Channel, (0~500V, 10A, 350W)

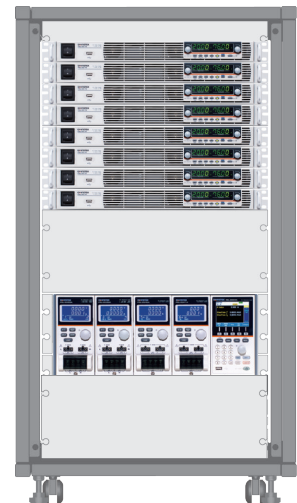

PSU series



Interface: USB, LAN, RS-232, GPIB(Optional)

maximum 4 units in parallel





※ Other interface does not use at LinkVieW.

PSU series provides maximum 2 units in series connection (models under 300V) to achieve maximum 600V or 4 units in parallel connection to obtain maximum 800A and the maximum output power of 6.24 kW.

	PSU6-200	PSU12.5-120	PSU20-76	PSU40-38	PSU60-25
V	6	12.5	20	40	60
A	200	120	76	38	25

	PSU100-15	PSU150-10	PSU300-5	PSU400-3.8	PSU600-2.6
V	100	150	300	400	600
A	15	10	5	3.8	2.6

4 channel Large Battery Charge / Discharge Test

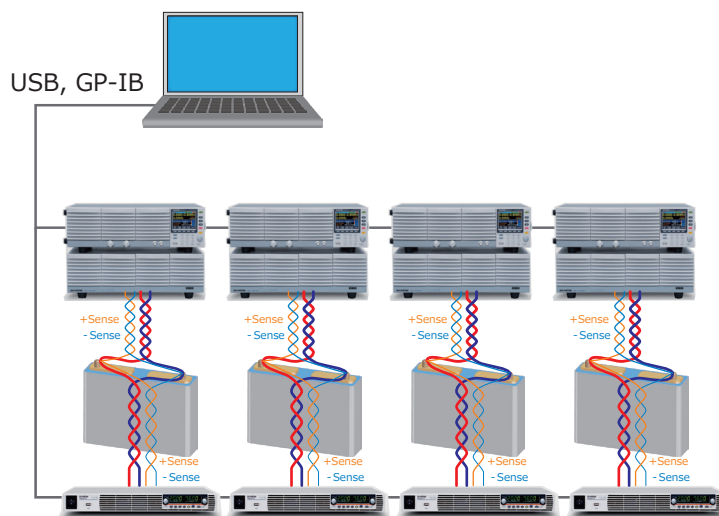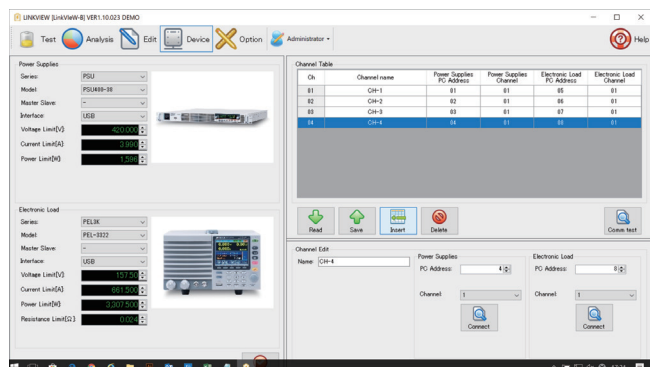

PEL-3000 series

PEL-3021



PEL-3111



PEL-3322



PEL-3533



PEL-3744



PEL-3955



Interface※: USB, RS-232, GPIB(Optional)

Model	PEL-3021	PEL-3041	PEL-3111	PEL-3211
Voltage	1.5V~150V	1.5V~150V	1.5V~150V	1.5V~150V
Current	35A	70A	210A	420A
Power	175W	350W	1050W	2100W

Model	PEL-3212	PEL-3323	PEL-3424	PEL-3535
Voltage	1.5V~150V	1.5V~150V	1.5V~150V	1.5V~150V
Current	0~420A	0~630A	0~840A	0~1050A
Power	2100W	3150W	4200W	5250W

Model	PEL-3322	PEL-3533	PEL-3744	PEL-3955
Voltage	1.5V~150V	1.5V~150V	1.5V~150V	1.5V~150V
Current	0~630A	0~1050A	0~1470A	0~1890A
Power	3150W	5250W	7350W	9450W

PSU series



Interface※: USB, LAN, RS-232, GPIB(Optional)
maximum 4 units in parallel



※ Other interface does not use at LinkVieW.

PSU series provides maximum 2 units in series connection (models under 300V) to achieve maximum 600V or 4 units in parallel connection to obtain maximum 800A and the maximum output power of 6.24 kW.

	PSU6-200	PSU12.5-120	PSU20-76	PSU40-38	PSU60-25
V	6	12.5	20	40	60
A	200	120	76	38	25

	PSU100-15	PSU150-10	PSU300-5	PSU400-3.8	PSU600-2.6
V	100	150	300	400	600
A	15	10	5	3.8	2.6